

# CaM Kinase IV KinEASE™ FP-645nm FarRed Assay

Catalog # 32-090

Sufficient reagents for two 384-well plates per kit.

<b>Contents</b>	<b>Page</b>
I. STORAGE AND STABILITY	2
II. ASSAY OVERVIEW	2
III. SYSTEM COMPONENTS	3
A. Provided Kit Components	3
B. Recommended Buffers	3
IV. ASSAY PROCEDURE	4
A. Kinase Reaction Module	4
B. Detection Module	5
V. APPENDIX A – Assay Optimization	7



sales orders 800 233 3991  
call collect from outside the u.s. 434 975 4300  
tech support 800 548 7853  
fax orders 866 831 3991  
www.upstate.com

**FOR IN VITRO RESEARCH USE ONLY.  
NOT RECOMMENDED OR INTENDED  
FOR DIAGNOSIS OF DISEASE IN  
HUMANS.**

**DO NOT USE IN HUMANS.**

## I. STORAGE AND STABILITY

**Storage:** Upon receipt, store individual components at recommended temperatures. Store the 384-well plates at room temperature. Store all other components at -20°C.


**Stability:** Components stable for 6 months from date of shipment if stored and handled correctly. We recommend that all enzymes to be used with this kit are stored as aliquots and a fresh aliquot used for each experiment.

## II. ASSAY OVERVIEW

In this assay, a phosphorylated peptide has been labeled with a red fluorescent dye. This phosphorylated tracer has a low molecular weight and thus a low fluorescence polarization value. The phosphorylated tracer binds to a phospho-specific antibody to form a high molecular weight complex with a high polarization value.

In a kinase reaction, a peptide or a protein substrate (non-fluorescently labeled) is phosphorylated by the kinase in the presence of ATP and Magnesium to form a phosphorylated product. This phosphorylated product competes with the tracer for binding to the phospho-specific antibody. As increasing amounts of phosphorylated product are formed from the kinase reaction, there is a reduction in the binding of tracer to antibody resulting in a decrease in the fluorescence polarization value.

CaM Kinase IV KinEASE™ FP-645nm FarRed Assay supplied in this kit offers a method for assaying CaM Kinase IV using preferred substrate and a generic detection system.

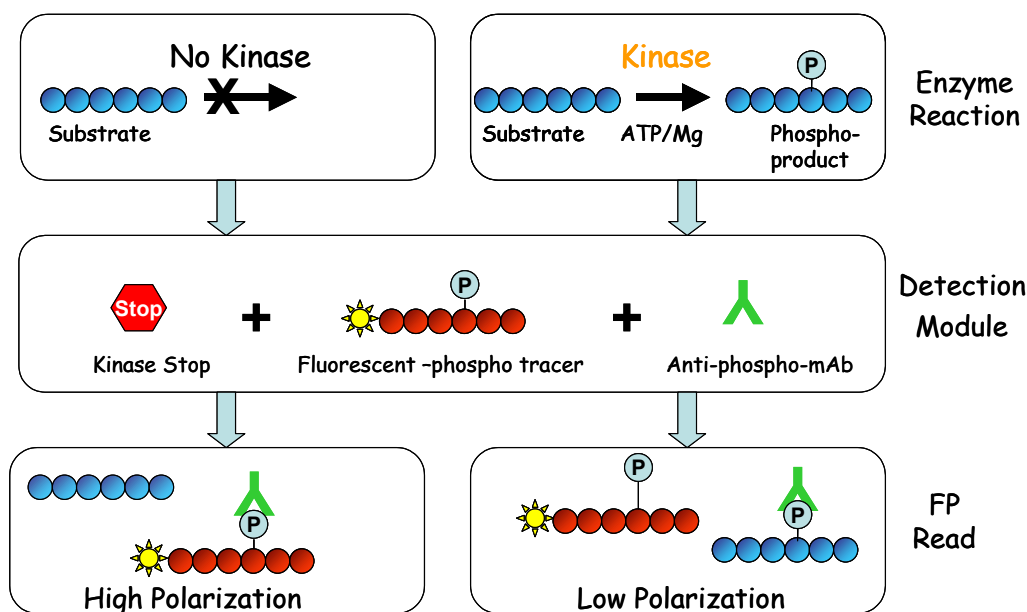

**Related Product:** CaM Kinase IV, Catalog # 14-547

### III. SYSTEM COMPONENTS

#### A. Provided Kit Components

Prior to use, each reagent should be vortexed, and then centrifuged to collect residual liquid trapped in the vial cap. **Please note the STK Tracer-red solution is light sensitive.**

Reagent	Catalog #	Stock	Volume Supplied	Storage
STK Substrate 1	12-548	10mM	120µl	-20°C
STK Antibody	35-002	20X	237µl	-20°C
STK Tracer-red	20-299	100X	48µl	-20°C
10X KinEASE™ Buffer	20-302	10X	5ml	-20°C
10X Detection Buffer	20-308	10X	3ml	-20°C
10X KinEASE™ Enzyme Dilution Buffer	2004306	10X	1ml	-20°C
MgCl <sub>2</sub>	20-303	1M	500µl	-20°C
DTT	20-265	1M	450µl	-20°C
CaCl <sub>2</sub>	20-305	10mM	0.5ml	-20°C
Calmodulin	14-368A	100µg	lyophilized	-20°C
ATP	20-306	10mM	300µl	-20°C
EDTA	20-307	0.5M	2ml	-20°C
384 Well KinEASE™ Plate	30-014		2 plates	RT

**Note:** Individual buffer components should be stored at -20°C until ready to use

#### B. Recommended Buffers

Buffer	5X Buffer
Reaction Buffer	250mM HEPES pH 7.2, 0.05% BSA (Probumin™, Chemicon Catalog # 3225-80), 25mM MgCl <sub>2</sub> , 500µM CaCl <sub>2</sub> , 1.25µM Calmodulin, 5mM DTT (DTT to be added immediately prior to use)
Detection Buffer	250mM HEPES pH 7.2, 0.5% Tween®-20, 5mM DTT (DTT to be added immediately prior to use)

Buffer	1X Buffer
Enzyme Dilution Buffer	50mM HEPES pH 7.2, 0.1% BSA (Probumin™, Chemicon Catalog # 1003512), 0.01% Brij-35, 0.1mM EDTA, 1mM DTT (DTT to be added immediately prior to use)

## IV. ASSAY PROCEDURE

**Safety Warnings and Precautions:** The CaM Kinase IV KinEASE™ FP-645nm FarRed Assay is designed for research use only. All chemicals should be considered potentially hazardous and principles of good laboratory practice should be followed.

### A. Kinase Reaction Module

Prepare sufficient volume of each solution based on the number of assays to be performed, plus a slight overage to account for pipetting inaccuracies (either 10-20% extra or one extra assay point is generally sufficient). **Note:** A precipitate may be observed in the thawed 0.5M EDTA (Catalog # 20-307). Warm the tube to 37°C for 15 minutes and vortex to bring into solution.

#### Reaction Solution Preparation

- 25µM Calmodulin:** Dilute 30µl 10X Reaction Buffer (20-302) to 300µl with water. Add 250µl to the lyophilized calmodulin.
- 5X Reaction Buffer:** For 1ml of 5X Reaction Buffer combine 370µl water, 500µl 10X KinEASE™ Buffer, 25µl 1M MgCl<sub>2</sub>, and 50µl 10mM CaCl<sub>2</sub>, 50µl 25µM Calmodulin, and 5µl 1M DTT. The total amount of 5X Reaction Buffer required will depend upon the number of experimental assay points. The 1ml volume should be scaled up (or down) according to the particular requirements of the experiment.
- 1X Reaction Buffer (for use in the No Enzyme Wells, Buffer Control Wells and Tracer Control Wells):** Prepare the 1X Reaction Buffer by diluting the 5X Reaction Buffer 5-fold with water (e.g., for 1ml of 1X Reaction Buffer combine 800µl water and 200µl 5X Reaction Buffer).
- 1X Enzyme Dilution Buffer (EDB):** For 1ml of the 1X EDB combine 899µl water, 100µl of 10X KinEASE™ Enzyme Dilution Buffer, and 1µl of 1M DTT. The 1ml volume should be scaled up (or down) according to the particular requirements of the experiment.
- 2.5X ATP Working Solution:** Prepare a 250µM ATP Working Solution in 1.25X Reaction Buffer (e.g., for 1ml of the 2.5X ATP Working Solution combine 725µl water, 250µl 5X Reaction Buffer, and 25µl 10mM ATP). 10µl of the 2.5X ATP Working Solution is required per well.
- 2.5X STK Substrate 1 Working Solution:** Prepare a 25µM STK Substrate 1 Working Solution in 1.25X Reaction Buffer (e.g., for 1ml of STK Substrate 1 Working Solution combine 747.5µl water, 250µl 5X Reaction Buffer and 2.5µl of 10mM STK Substrate 1). 10µl of 2.5X STK Substrate 1 Working Solution is required per well.
- 5X CaM Kinase IV Working Solution:** Prepare the CaM Kinase IV Working Solution in 1X KinEASE™ EDB at a concentration of 5X the required final reaction concentration. 5µl of CaM Kinase IV Working Solution is required per well.

#### Reaction Protocol

- Set up 3 assay controls as detailed below.

**Buffer Control Wells (assay background)**

25µl 1X Reaction Buffer

**Tracer Control Wells (min. mP value)**

25µl 1X Reaction Buffer

**No Enzyme Wells (max. mP value)**

10µl STK Substrate 1 Working Solution

5µl 1X Reaction Buffer

10µl ATP Working Solution

- Set up reactions as detailed below.

#### Plus Enzyme Wells

10µl STK Substrate 1 Working Solution  
 5µl CaM Kinase IV Working Solution  
 10µl ATP Working Solution

The reactions are started by addition of the 10µl ATP Working Solution. When using the same concentration of enzyme (e.g. EC<sub>70</sub> value), the substrate working solution and enzyme working solutions can be combined and added as 15µl per well.

If required, 0.5µl DMSO may be added to a set of control wells to simulate compound addition.

- Incubate reactions for the required length of time at the appropriate temperature. To ensure that all reaction components have collected in the bottom of the wells, very gently tap the bottom of the plate against the bench top. **Note:** Optimum kinase reaction incubation time and temperature should be determined by the end user. Typical kinase reaction conditions used at Upstate are 30-60 minutes at room temperature with constant agitation.

## B. Detection Module

### Detection Solution Preparation

- 5X Detection Buffer:** Prepare the 5X Detection Buffer by diluting the 10X Detection Buffer 2-fold and adding DTT to a concentration 5mM (e.g. for 1ml of 5X Detection Buffer combine 495µl water, 500µl of 10X KinEASE™ Buffer and 5µl of 1M DTT).
- 1X Detection Buffer (for use in the Buffer Control Wells and Tracer Control Wells):** Prepare the 1X Detection Buffer by diluting the 5X Detection Buffer 5-fold with water (e.g., for 1ml of 1X Detection Buffer add 200µl 5X Detection Buffer to 800µl water).
- STK Stop Mix:** Prepare STK Stop Mix containing STK Tracer-red and EDTA in 1X Detection Buffer by diluting the STK Tracer-red 100-fold and adding EDTA to a concentration of 140mM (e.g., for 1ml of STK Stop Mix combine 510µl water, 280µl 0.5M EDTA pH 7.2, 200µl 5X Detection Buffer and 10µl 100X STK Tracer-red). 5µl of STK Stop Mix is required per well.
- STK Antibody Mix:** Prepare STK Antibody Mix containing STK Antibody in 1X Detection Buffer by diluting the STK Antibody 20-fold (e.g., for 1ml of STK Antibody Mix combine 750µl water, 200µl 5X Detection Buffer and 50µl 20X STK Antibody). 5µl of 5X STK Antibody Mix is required per well.

### Detection Protocol

- Add the following to the 3 sets of assay controls wells.

#### Buffer Control Wells (assay background)

10µl 1X Detection Buffer

#### Tracer Control Wells (min. mP value)

5µl of STK Stop Mix  
 5µl 1X Detection Buffer

#### No Enzyme Wells (max. mP value)

5µl STK Stop Mix  
 5µl STK Antibody Mix

- Stop the reactions by adding 5µl/well STK Stop Mix.
- Add 5µl/well STK Antibody Mix. **Note:** Once the STK Stop Mix has been added to the Tracer Control wells, the STK Stop Mix and STK Antibody Mix may be combined and added as 10µl/well.

4. Incubate the plate for a minimum of 4 hours at room temperature (assay signal is stable for up to 24 hours).
4. Read plate on a Fluorescence Polarization Reader. The end user must optimize their instrument parameters for optimal assay sensitivity. Recommended parameters for the MDC Analyst AD used at Upstate are as follows:

**Method:** *Fluorescence Polarization*  
**Excitation:** 560AF55  
**Emission:** 645AF75  
**Mirror:** 595DRLP  
**Lamp:** *Continuous*  
**Z-height:** 3mm (to be determined for individual readers)  
**Readings per well:** 1  
**Integration time:** 100000 $\mu$ sec

**Attenuator:** *out*  
**PMT setup:** *Smartread Sensitivity 2*  
**Excitation Polarizer:** *S (static)*  
**Emission Polarizer:** *SP (dynamic)*  
**G Factor:** (to be determined for individual readers)  
Select Buffer Control Wells for background subtraction.

### **General Assay Notes**

- It is recommended that the MgCl<sub>2</sub> final reaction concentration should not exceed 5mM in the reaction (*i.e.*, 25mM in the 5X Reaction Buffer). If a higher concentration of MgCl<sub>2</sub> is required then do not exceed 10mM MgCl<sub>2</sub> (*i.e.*, 50mM in the 5X Reaction Buffer) and run an enzyme reaction with stop mix and Antibody mix added prior to ATP addition to confirm that the reaction is stopped under these conditions.
- The 10X KinEASE™ Buffer (Catalog # 20-302) is used to prepare 5X working stocks to ensure a final 1X buffer concentration in the assay. These working buffers should be stored at 4°C until ready to use. If long-term storage (one week to six months) is required, DTT should be omitted until assay is to be performed and sodium azide added to the 5X buffer at a final concentration of 0.05%.

## V. APPENDIX A - Assay Optimization

### Determination of Enzyme Concentration for Screening

Using the optimized assay conditions, a suitable enzyme concentration for screening applications may then be determined by following the procedure outlined below.

Set up an enzyme titration with two-fold serial dilutions of enzyme and appropriate controls (No Enzyme Wells, Tracer Control Wells and Buffer Control Wells) according to the standard assay protocol.

Analyze the results obtained by plotting a graph of enzyme concentration (Units/ml) vs. Fluorescence Polarization (mP) (see below for example).

Determine the EC<sub>70</sub> mP using the following formula:

$$EC_{70} \text{ mP} = ((\text{No Enzyme Control} - \text{Tracer Control}) \times 0.3) + \text{Tracer Control}$$

From the graph of enzyme concentration (Units/ml) vs. Fluorescence Polarization (mP) determine the concentration of enzyme that correlates to the EC<sub>70</sub> mP value calculated above. This enzyme concentration (EC<sub>70</sub> Units/ml) is recommended for screening applications.

