

KinEase FP Assay

Module 1 – Serine/Threonine Kinases

Catalog # 32-001

Lot # 28308U

Sufficient reagents for two 384-well plates per kit.

Contents	Page
I. STORAGE AND STABILITY	2
II. ASSAY OVERVIEW	2
III. SYSTEM COMPONENTS	3
A. Provided Kit Components	3
B. Required Materials Not Provided	3
C. Recommended Buffers	4
IV. ASSAY PROCEDURE	4
A. Preparation of Assay Solutions	4
B. Protocol	5
V. APPENDIX A – Assay Optimization	6
VI. APPENDIX B – Recommended Reaction Conditions	8



sales orders 800 233 3991
call collect from outside the u.s. 434 975 4300
tech support 800 548 7853
fax orders 866 831 3991
www.upstate.com

**FOR IN VITRO RESEARCH USE ONLY.
NOT RECOMMENDED OR INTENDED
FOR DIAGNOSIS OF DISEASE IN
HUMANS.**

DO NOT USE IN HUMANS.

I. STORAGE AND STABILITY

Storage: Upon receipt, all reagents should be stored at -20°C.

Stability: Components stable for 6 months from date of shipment if stored and handled correctly. We recommend that all enzymes to be used with this kit are stored as aliquots and a fresh aliquot used for each experiment.

II. ASSAY OVERVIEW


In this assay a phosphorylated peptide has been labeled with a green fluorescent dye. This phosphorylated tracer has a low molecular weight and thus a low fluorescence polarization value. The phosphorylated tracer binds to a phospho-specific antibody to form a high molecular weight complex with a high polarization value.

In a kinase reaction a peptide or a protein substrate (non-fluorescently labeled) is phosphorylated by the kinase in the presence of ATP and Magnesium to form a phosphorylated product. This phosphorylated product competes with the tracer for binding to the phospho-specific antibody. As increasing amounts of phosphorylated product are formed from the kinase reaction, there is a reduction in the binding of tracer to antibody resulting in a decrease in the fluorescence polarization value.

KinEase FP Assay Module 1 supplied in this kit offers a method for assaying Serine/Threonine kinases using three potential substrates and a generic detection system. It has been designed to allow the user to evaluate the application of the technology to their own kinase.

KinEase FP Assay Module 1 is known to work with the following enzymes: **AMPK (r), Aurora A (h), CaM Kinase II (r), CaM Kinase IV (h), CHK1 (h), CHK2 (h), IKK α (h), IKK β (h), MAPKAP Kinase 2 (h), MSK1 (h), p70 S6 Kinase (h), PAK2 (h), Pim1 (h), PKA (h), Akt1/PKB α (h), Akt2/PKB β (h), Akt3/PKB γ (h), PKC α (h), PKC β I (h), PKC β II (h), PKC γ (h), PKC δ (h), PKC ϵ (h), PKC eta (h), PKC iota (h), PKC μ (h), PKC theta (h), PKC zeta (h), PKD2 (h), PRAK (h), PRK2 (h), ROK α /ROCK-II (h), Rsk1/MAPKAP Kinase 1a (h), Rsk1/MAPKAP Kinase 1a (r), Rsk2/MAPKAP Kinase 1b (h), Rsk3 (h) and SGK1 (h)** (see Appendix B for further details).

h = human; r = rat

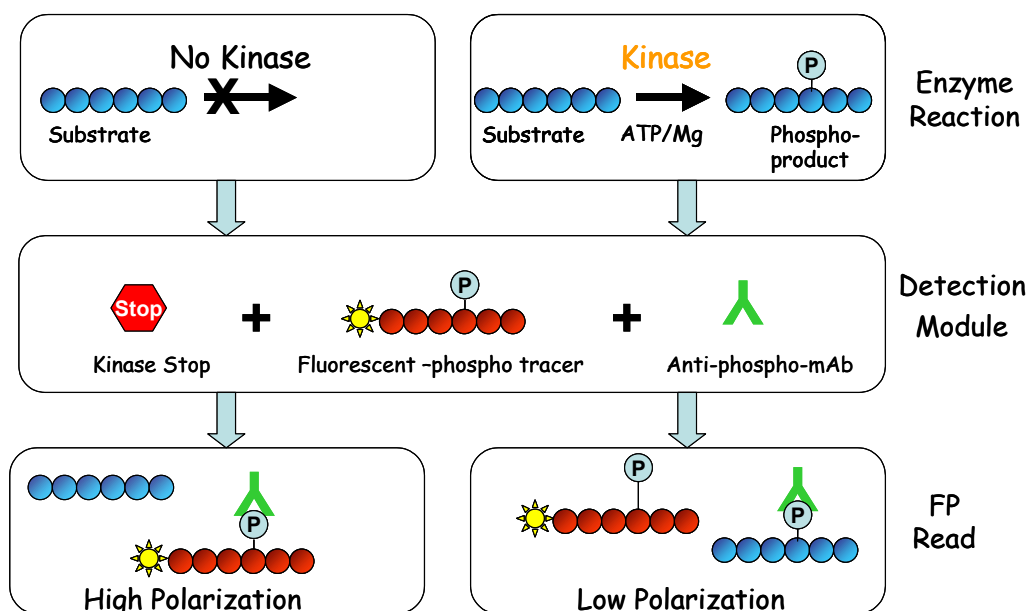

III. SYSTEM COMPONENTS

A. Provided Kit Components

Prior to use, each reagent should be vortexed, then centrifuged to collect residual liquid trapped in the vial cap. **Please note the STK Tracer solution is light sensitive.**

Reagent	Catalog #	Lot #	Stock	Volume Supplied	Storage
STK Substrate 1	12-548	28258U	10mM	58µl	-20°C
STK Substrate 2	12-549	28259U	10mM	58µl	-20°C
STK Substrate 3	12-550	28260U	10mM	58µl	-20°C
STK Antibody	35-002	28275U	20X	192µl	-20°C
STK Tracer	20-287	28261U	100X	38µl	-20°C

B. Required Materials Not Provided

Reagent	Recommended Supplier	Stock	Storage
ATP	Major Laboratory Suppliers	100mM	Store aliquoted -20°C
DTT	Major Laboratory Suppliers	1M	Store aliquoted -20°C
BSA	Sigma A2934	1% in water	Store aliquoted -20°C
EDTA	Major Laboratory Suppliers	0.5M pH 7.2	RT
MgCl ₂	Major Laboratory Suppliers	1M	RT
HEPES	Major Laboratory Suppliers	1M	RT
Black 384 well microplates	Costar 3710		RT
Water (18.2MΩ)			RT

C. Recommended Buffers

Buffers should be prepared as 5X stocks to ensure a final 1X buffer concentration in the assay. These buffers should be stored at 4°C. If long-term storage (one week to six months) is required, sodium azide should be added to the 5X buffer at a final concentration of 0.05%. See Appendix B for recommended 1X Reaction Buffer conditions for the Upstate kinases listed on page 2.

Buffer	5X Buffer
Reaction Buffer*	250mM HEPES pH 7.2, 25mM MgCl ₂ , 0.05% BSA
Detection Buffer	250mM HEPES pH 7.2, 0.05% BSA, 5mM DTT (DTT to be added immediately prior to use)

*Other components that may be added to the Reaction Buffer if required are MnCl₂, CaCl₂, Calmodulin, DTT, AMP, Lipid activator (Upstate Catalog # 20-133) or β-mercaptoethanol.

It is recommended that the MgCl₂ final reaction concentration should not exceed 5mM in the reaction (*i.e.*, 25mM in the 5X Reaction Buffer). If a higher concentration of MgCl₂ is required then do not exceed 10mM MgCl₂ (*i.e.*, 50mM in the 5X Reaction Buffer) and run an enzyme reaction with stop mix and detection mix added prior to ATP addition to confirm that the reaction is stopped under these conditions.

IV. ASSAY PROCEDURE

Safety Warnings and Precautions: The KinEase FP Assay is designed for research use only. All chemicals should be considered potentially hazardous and principles of good laboratory practice should be followed.

A. Preparation of Assay Solutions

Prepare sufficient volume of each solution based on the number of assays to be performed, plus a slight overage to account for pipetting inaccuracies (either 10% extra or one extra assay point is generally sufficient).

Reaction Component Preparation

- 1X Reaction Buffer (for use in the No Enzyme Wells, Buffer Control Wells and Tracer Control Wells):** Prepare the 1X Reaction Buffer by diluting the 5X Reaction Buffer 5-fold with water (*e.g.*, for 1ml of 1X Reaction Buffer combine 800μl water and 200μl 5X Reaction Buffer).
- ATP Working Solution:** Prepare the ATP Working Solution in 1X Reaction Buffer at an ATP concentration of 2.5X the required final reaction concentration (*e.g.*, for a 100μM final reaction concentration prepare a 250μM ATP Working Solution by combining ATP, 5X Reaction Buffer and water). 10μl of ATP Working Solution is required per well.
- STK Substrate Working Solution:** For each substrate to be tested prepare a 150μM STK Substrate Working Solution in Reaction Buffer. This is 5X the required assay concentration of 30μM (*e.g.*, to prepare 1ml of STK Substrate Working Solution combine 785μl water, 200μl 5X Reaction Buffer and 15μl of 10mM STK Substrate). 5μl of STK Substrate Working Solution is required per well.
- Kinase Working Solution:** Prepare the Kinase Working Solution in 1X Reaction Buffer at a concentration of 2.5X the required final reaction concentration. 10μl of Kinase Working Solution is required per well.

Detection Component Preparation

- 1X Detection Buffer (for use in the Buffer Control Wells and Tracer Control Wells):** Prepare the 1X Detection Buffer by diluting the 5X Detection Buffer 5-fold with water (e.g., for 1ml of 1X Detection Buffer add 200 μ l 5X Detection Buffer to 800 μ l water).
- STK Stop Mix:** Prepare STK Stop Mix containing STK Tracer and EDTA in 1X Detection Buffer by diluting the STK Tracer 100-fold and adding EDTA to a concentration of 140mM (e.g., for 1ml of STK Stop Mix combine 510 μ l water, 280 μ l 0.5M EDTA pH 7.2, 200 μ l 5X Detection Buffer and 10 μ l 100X STK Tracer). 5 μ l of STK Stop Mix is required per well.
- STK Detection Mix:** Prepare a STK Detection Mix containing STK Antibody in 1X Detection Buffer by diluting the STK Antibody 20-fold (e.g., for 1ml of STK Detection Mix combine 750 μ l water, 200 μ l 5X Detection Buffer and 50 μ l 20X STK Antibody). 5 μ l of STK Detection Mix is required per well.

B. Protocol

- Set up Reactions as detailed below.

No Enzyme Wells

5 μ l STK Substrate Working Solution
 10 μ l 1X Reaction Buffer
 10 μ l ATP Working Solution

Plus Enzyme Wells

5 μ l STK Substrate Working Solution
 10 μ l Kinase Working Solution
 10 μ l ATP Working Solution

(The reactions are started by addition of the 10 μ l ATP Working Solution).

If required, 0.5 μ l DMSO may be added to the well to simulate compound addition.

- Incubate reactions for required length of time at room temperature.
- Stop the reactions by adding 5 μ l/well STK Stop Mix.
- Add 5 μ l/well STK Detection Mix. **Note:** STK Stop Mix and STK Detection Mix may be combined and added as 10 μ l/well.

The following control wells should be set up for each experiment

Buffer Control Wells

25 μ l 1X Reaction Buffer
 10 μ l 1X Detection Buffer

Tracer Control Wells

25 μ l 1X Reaction Buffer
 5 μ l STK Stop Mix
 5 μ l 1X Detection Buffer

- Incubate the plate for a minimum of 4 hours at room temperature (assay signal is stable for up to 24 hours).
- Read plate on a Fluorescence Polarization Reader. Recommended parameters for the MDC Analyst AD are as follows:

Method: *Fluorescence Polarization*
Excitation: 485nm (bw20)
Emission: 530nm (bw25)
Mirror: Dichroic 505
Lamp: *Continuous*
Zheight: 3mm (to be determined for individual readers)
Readings per well: 1
Integration time: 100000 μ sec


Attenuator: *out*
PMT setup: *Smartread Sensitivity 3*
Excitation Polarizer: *S (static)*
Emission Polarizer: *SP (dynamic)*
G Factor: (to be determined for individual readers)
 Select Buffer Control Wells for background subtraction.

V. APPENDIX A - Assay Optimization

Substrate Selection

To determine whether KinEase FP Assay Module 1 is suitable for your kinase, a series of enzyme dilutions should be tested with each STK Substrate (30 μ M final reaction concentration) according to the standard assay protocol.

The following graph shows data obtained from titration of a Ser/Thr Kinase with STK Substrates 1, 2 and 3. Enzyme activity is observed as a decrease in the Fluorescence Polarization (mP) and in the example given STK Substrate 1 was optimal.

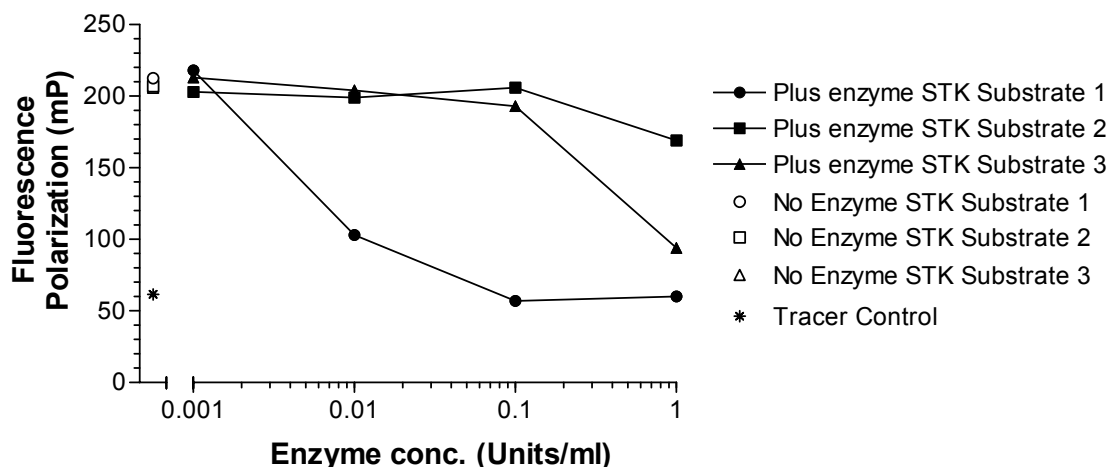

Once enzyme activity has been demonstrated it is recommended the user optimize their reaction conditions (i.e. substrate concentration and reaction buffer constituents) to maximize the assay sensitivity. See Appendix B for recommended conditions for the Upstate kinases listed on page 2.

Determination of Enzyme Concentration for Screening

Using the optimized assay conditions, a suitable enzyme concentration for screening applications may then be determined by following the procedure outlined below.


Set up an enzyme titration with two-fold serial dilutions of enzyme and appropriate controls (No Enzyme Wells, Tracer Control Wells and Buffer Control Wells) according to the standard assay protocol.

Analyze the results obtained by plotting a graph of enzyme concentration (Units/ml) vs. Fluorescence Polarization (mP) (see below for example).

Determine the EC₇₀ mP using the following formula:

$$EC_{70} \text{ mP} = ((\text{No Enzyme Control} - \text{Tracer Control}) \times 0.3) + \text{Tracer Control}$$

From the graph of enzyme concentration (Units/ml) vs. Fluorescence Polarization (mP) determine the concentration of enzyme that correlates to the EC₇₀ mP value calculated above. This enzyme concentration (EC₇₀ Units/ml) is recommended for screening applications.

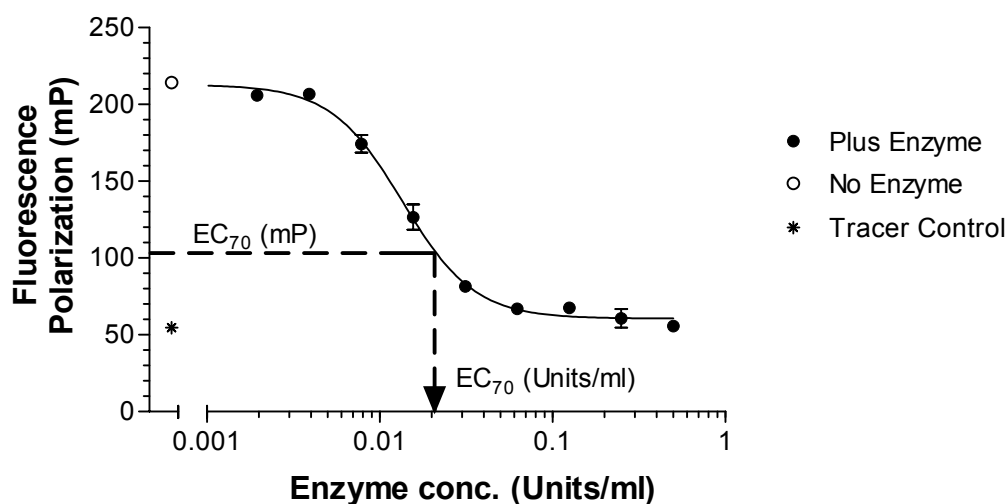

VI. APPENDIX B – Recommended Reaction Conditions

Table of recommended reaction conditions for Upstate kinases (h = human; r = rat):

Kinase (Catalog #)	Recommended Substrate	Recommended Substrate Conc.	Recommended 1X Reaction Buffer
AMPK (r) (14-305)	STK Substrate 1	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 50 μ M AMP
Aurora A (h) (14-511)	STK Substrate 2	200 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
CaM Kinase II (r) (14-217)	STK Substrate 1	10 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT, 100 μ M CaCl ₂ , 250nM Calmodulin
CaM Kinase IV (h) (14-547)	STK Substrate 1	10 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT, 100 μ M CaCl ₂ , 250nM Calmodulin
CHK1 (h) (14-346)	STK Substrate 1	10 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
CHK2 (h) (14-347)	STK Substrate 1	200 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
IKK α (h) (14-461)	STK Substrate 1	200 μ M	50mM HEPES pH 7.2, 0.01% BSA, 2mM MgCl ₂ , 1mM DTT
IKK β (h) (14-485)	STK Substrate 1	200 μ M	50mM HEPES pH 7.2, 0.01% BSA, 2mM MgCl ₂ , 1mM DTT
MAPKAP Kinase 2 (h) (14-337)	STK Substrate 1	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
MSK1 (h) (14-548)	STK Substrate 3	10 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
p70 S6 Kinase (h) (14-486)	STK Substrate 3	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 2mM MgCl ₂ , 1mM DTT
PAK2 (h) (14-481)	STK Substrate 2	200 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
Pim1 (h) (14-573)	STK Substrate 3	200 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
PKA (h) (14-440)	STK Substrate 2	10 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
Akt1/PKB α (h) (14-276)	STK Substrate 3	10 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
Akt2/PKB β (h) (14-339)	STK Substrate 3	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
Akt3/PKB γ (h) (14-502)	STK Substrate 3	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
PKC α (h) (14-484)	STK Substrate 1	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 10mM MgCl ₂ , 1mM DTT, 1X Lipid Activator

Kinase	Recommended Substrate	Recommended Substrate Conc.	Recommended 1X Reaction Buffer
PKC β I (h) (14-503)	STK Substrate 1	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 10mM MgCl ₂ , 1mM DTT, 1X Lipid Activator
PKC β II (h) (14-496)	STK Substrate 1	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT, 1X Lipid Activator
PKC γ (h) (14-483)	STK Substrate 1	100 μ M	50mM HEPES pH 7.2, 0.01% BSA, 10mM MgCl ₂ , 1mM DTT, 1X Lipid Activator
PKC δ (h) (14-504)	STK Substrate 1	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 10mM MgCl ₂ , 1mM DTT, 1X Lipid Activator
PKC ϵ (h) (14-518)	STK Substrate 1	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 10mM MgCl ₂ , 1mM DTT, 1X Lipid Activator
PKC eta (h) (14-497)	STK Substrate 1	100 μ M	50mM HEPES pH 7.2, 0.01% BSA, 10mM MgCl ₂ , 1mM DTT, 1X Lipid Activator
PKC iota (h) (14-505)	STK Substrate 1	200 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
PKC μ (h) (14-508)	STK Substrate 1	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
PKC theta (h) (14-444)	STK Substrate 1	200 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
PKC zeta (h) (14-525)	STK Substrate 1	200 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
PKD2 (h) (14-506)	STK Substrate 1	200 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
PRAK (h) (14-334)	STK Substrate 1	100 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
PRK2 (h)	STK Substrate 1	10 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
ROK α /ROCK-II (h) (14-451)	STK Substrate 2	100 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
Rsk1/MAPKAP Kinase 1a (h) (14-509)	STK Substrate 1	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
Rsk1/MAPKAP Kinase 1a (r) (14-479)	STK Substrate 1	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
Rsk2/MAPKAP Kinase 1b (h) (14-480)	STK Substrate 1	30 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
Rsk3 (h) (14-462)	STK Substrate 1	200 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT
SGK1 (h) (14-331)	STK Substrate 3	10 μ M	50mM HEPES pH 7.2, 0.01% BSA, 5mM MgCl ₂ , 1mM DTT