

---

## Certificate of Analysis

**Catch and Release<sup>®</sup> v2.0**  
(Reversible Immunoprecipitation System)  
Catalog # 17-500A  
Lot # 33378

### Kit Components

**Antibody Capture Affinity Ligand**, Catalog # 20-216A. One vial containing **6 $\mu$ g** Antibody Capture Affinity Ligand in **60 $\mu$ l** PBS containing 2mM PMSF and 10% glycerol. Store at 4°C.

**Catch and Release<sup>®</sup> Wash Buffer, 10X**, Catalog # 20-210A. One vial containing **1.5ml** of 10X buffer, pH 7.4 containing the following detergents: 10% NP-40, 2.5% deoxycholic acid and 150mM imidazole. Store at 4°C. **Note:** If crystallization occurs when buffer is stored at 4°C, warm to room temperature and vortex briefly before use.

**Catch and Release<sup>®</sup> Non-denaturing Elution Buffer, 4X**, Catalog # 20-209A. One vial containing **1ml** of 4X PBS-based IP Elution Buffer. Store at 4°C.

**Catch and Release<sup>®</sup> Denaturing Elution Buffer, 1X**, Catalog # 20-284A. One vial containing **0.5ml** of 1X Tris-based IP Elution Buffer. Add  $\beta$ -mercaptoethanol (BME) to a final concentration of 5% v/v immediately before use. Store at 4°C.

**Catch and Release<sup>®</sup> v2.0 Spin Columns**, Catalog # 20-285. **5 columns** containing 0.5ml of prepacked IP capture resin. Store at 4°C

**Catch and Release<sup>®</sup> Capture Tubes**. Ten, 2ml reservoir tubes.

**FOR RESEARCH USE ONLY  
NOT FOR USE IN HUMANS**

---

### Kit Description


**Quantity:** 5 Immunoprecipitations per kit.

**Storage and Stability:** All components to be stored at 4°C. Components are stable for 6 months from date of shipment.

**Use:** This kit allows for quick and reproducible immunoprecipitation (IP) by using a spin column. The system is more reproducible than regular IP's, which are problematic with regards to washing the protein A/G agarose without disrupting the agarose bed. The binding of the antibody/antigen complex in Catch and Release<sup>®</sup> is reversible, and elution of the immune complex can occur with native or denaturing buffers. The system has been tested successfully with rabbit, mouse, sheep and goat antibodies. IP using human IgG1-4 should be suitable. IP using chicken antibodies or human IgA, IgD, IgE or IgM is not recommended with this kit. Please read the enclosed product manual before use.


---

**Quality Control Testing**

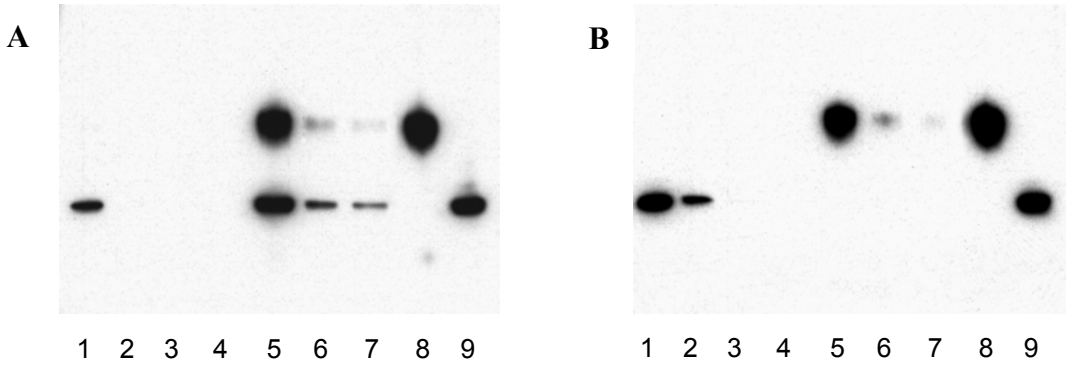

**Catch and Release<sup>®</sup> with Denaturing Elution Buffer:**

Catch and Release<sup>®</sup> columns and protocol were used with the Denaturing Elution Buffer to immunoprecipitate cdk2. HeLa nuclear extract was mixed with A. Anti-cdk2 (Catalog # 06-505) or B. normal, rabbit IgG as a negative control for 1 hour at room temperature. Samples from each fraction were run on an SDS-PAGE gel and immunoblotted. The upper band is the heavy chain of IgG and the lower band is cdk2. Lane 1: flow through; Lane 2: wash 1; Lane 3: wash 2; Lane 4: wash 3; Lane 5: elution 1; Lane 6: elution 2; Lane 7: elution 3; Lane 8: Anti-cdk2; Lane 9: HeLa nuclear extract.

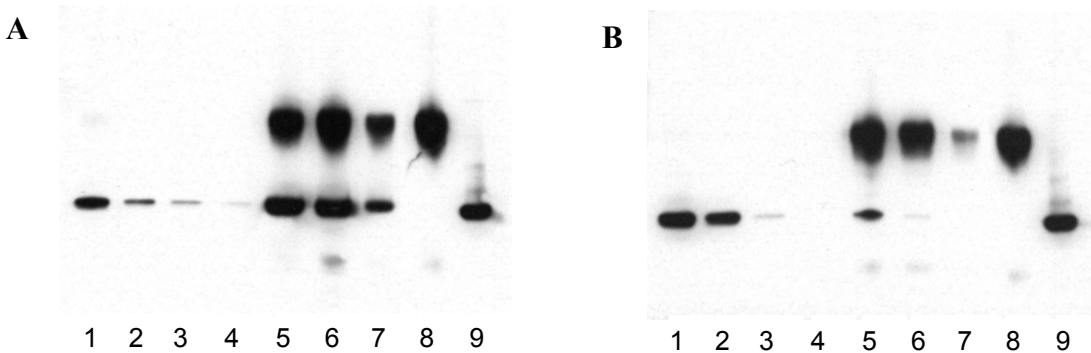

**Catch and Release<sup>®</sup> with Non-denaturing Elution Buffer:**

Catch and Release<sup>®</sup> columns and protocol were used with the Non-denaturing Elution Buffer to immunoprecipitate cdk2. HeLa nuclear extract was mixed with A. Anti-cdk2 (Catalog # 06-505) or B. normal, rabbit IgG as a negative control for 1 hour at room temperature. Samples from each fraction were run on an SDS-PAGE gel and immunoblotted. The upper band is the heavy chain of IgG and the lower band is cdk2. Lane 1: flow through; Lane 2: wash 1; Lane 3: wash 2; Lane 4: wash 3; Lane 5: elution 1; Lane 6: elution 2; Lane 7: elution 3; Lane 8: Anti-cdk2; Lane 9: HeLa nuclear extract.